MICROSCOPE: A Software System for Multivariate Analysis

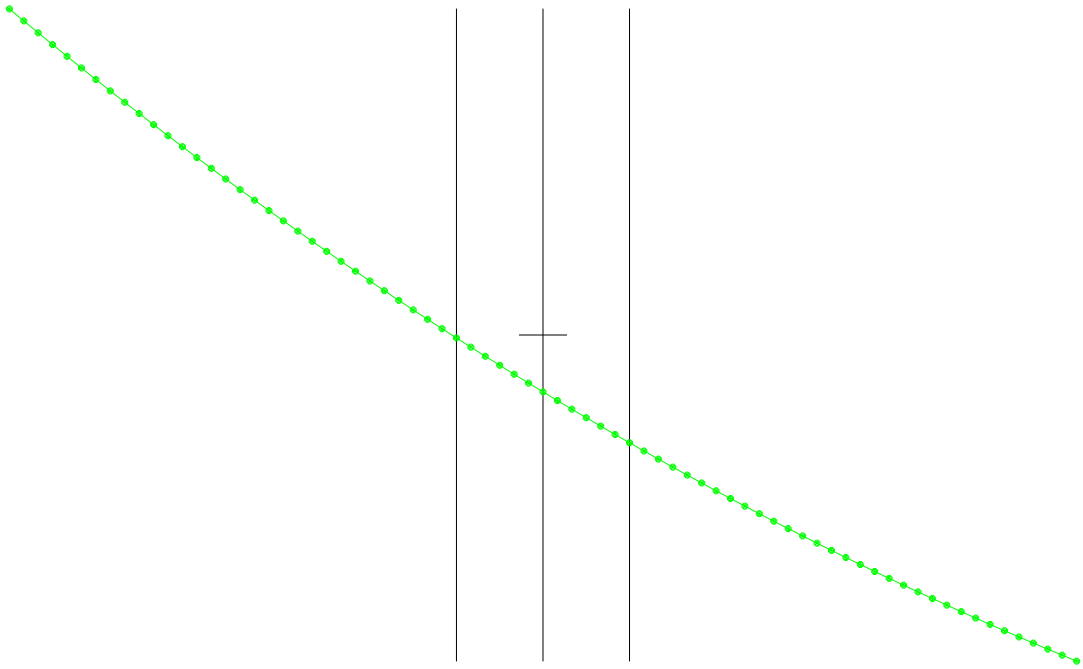

Point = 0.0
Direction = 1.000
F0 • (−0.02028, 0.02884)

s = 2.50E−03
h = 0.0150
Number of Evaluations: 287

This plot corresponding to figure

3