MICROSCOPE: A Software System for Multivariate Analysis

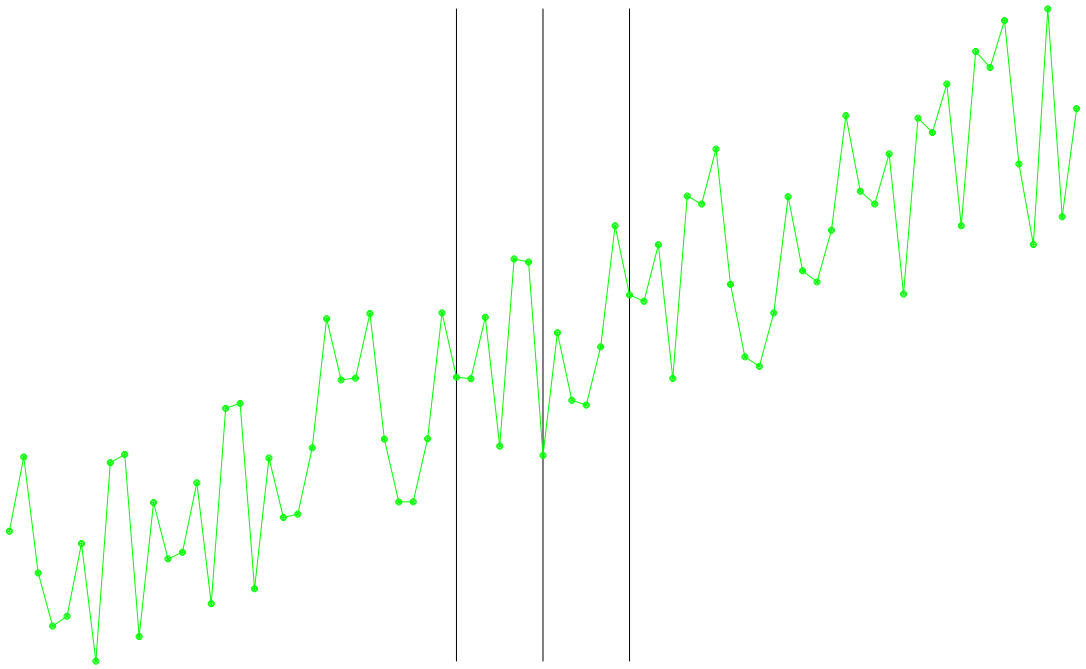

Point = 0.234
Direction = 1.000
F0 • (2.163E-10, 7.315E-10)

s = 2.50E-03
h = 0.0150
Number of Evaluations: 742

This plot corresponding to figure

10