MICROSCOPE: A Software System for Multivariate Analysis

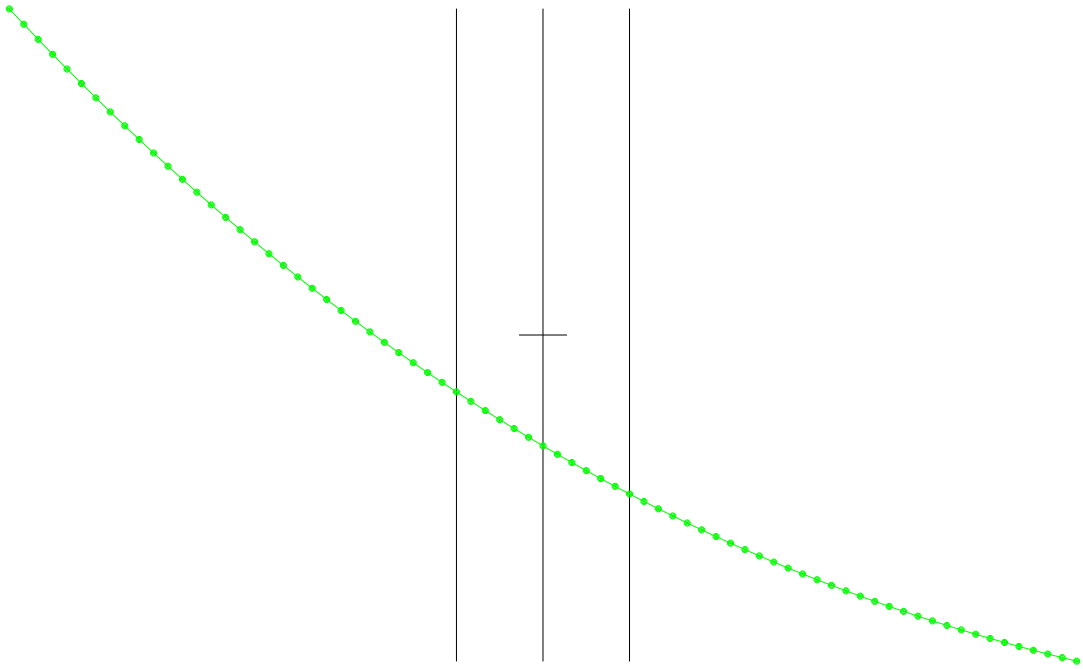

Point = 0.0
Direction = 1.000
F0 • (−0.03333, 0.06765)

s = 5.00E−03
h = 0.0300
Number of Evaluations: 249

This plot corresponding to figure

2