MICROSCOPE: A Software System for Multivariate Analysis

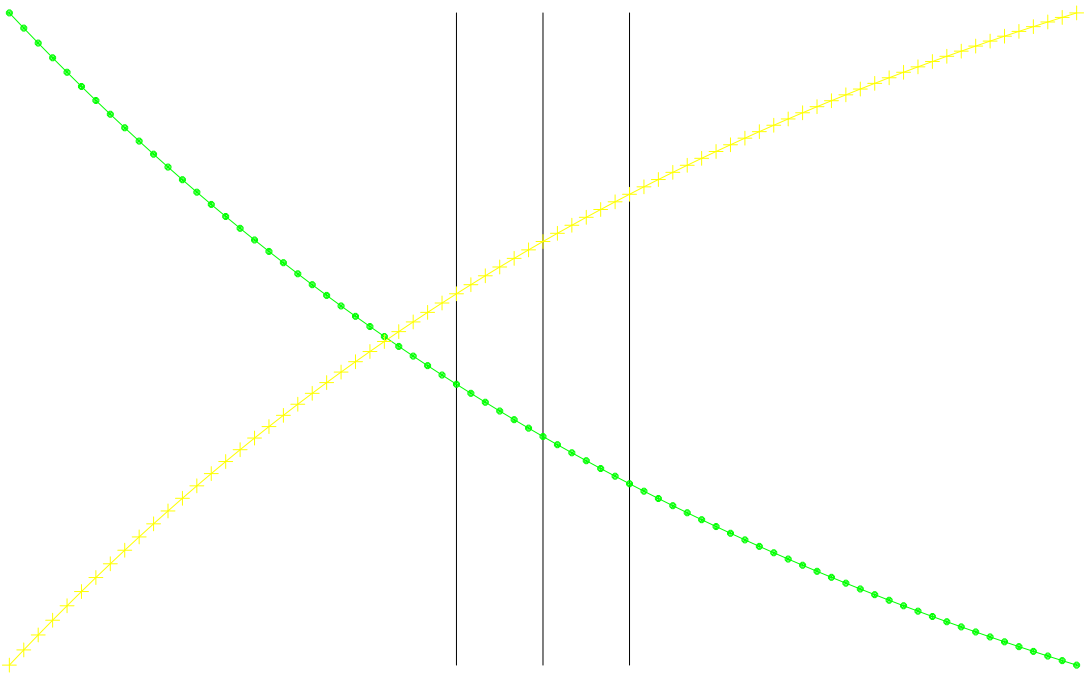

Point = 0.0
Direction = −1.000
F0 • (0.5397, 1.853)
Number of Evaluations: 2424

s = 0.0167
h = 0.1000
F1 + (−1.856, −0.5406)

This plot corresponding to figure

26