MICROSCOPE: A Software System for Multivariate Analysis

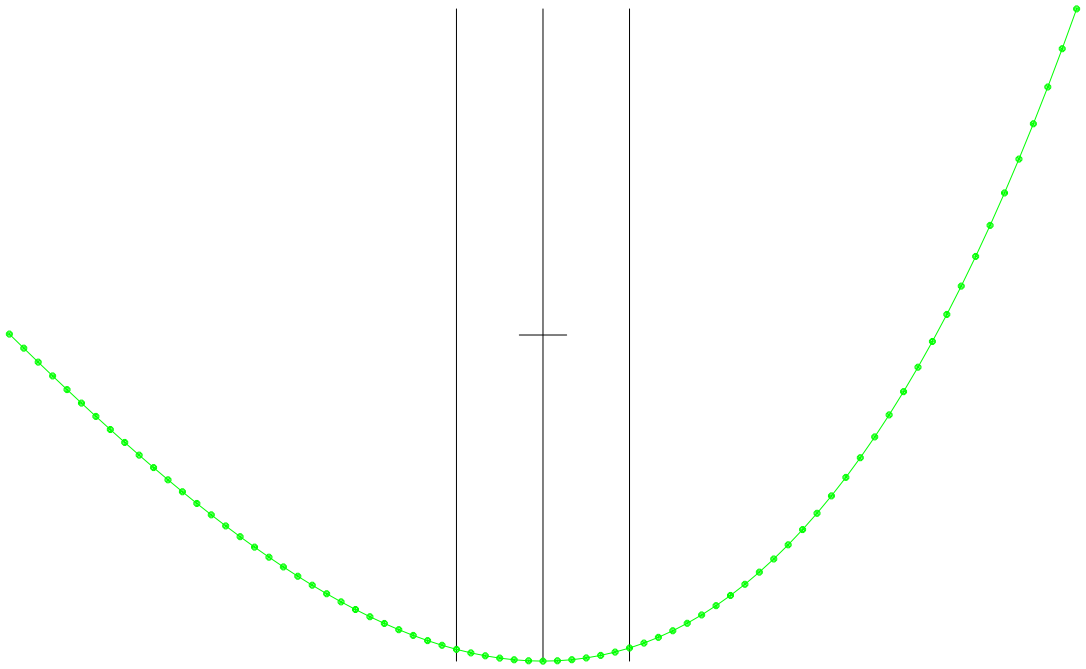

Point = 2.00
Direction = 1.000
F0 • (2.640E-11, 0.01416)

s = 5.00E-03
h = 0.0300
Number of Evaluations: 362

This plot corresponding to figure

4