MICROSCOPE: A Software System for Multivariate Analysis

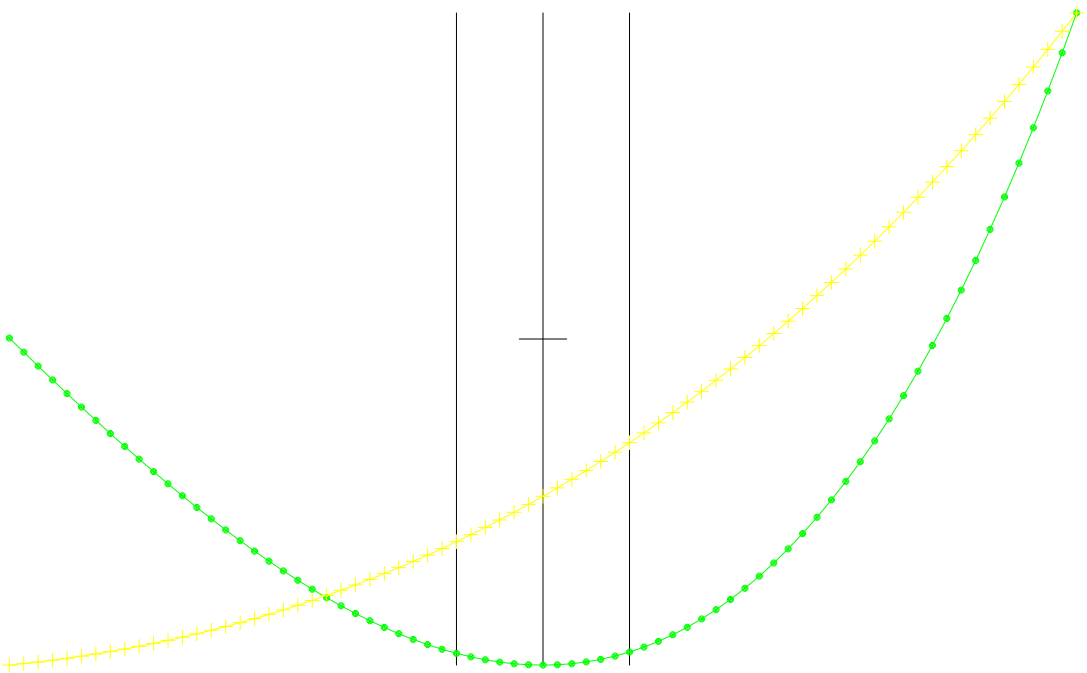

Point = 2.00 s = 5.00E-03
Direction = 1.000 h = 0.0300
F0 • (2.640E-11, 0.01416) F1 + (-0.06112, 0.1769)
Number of Evaluations: 374

This plot corresponding to figure

5