MICROSCOPE: A Software System for Multivariate Analysis

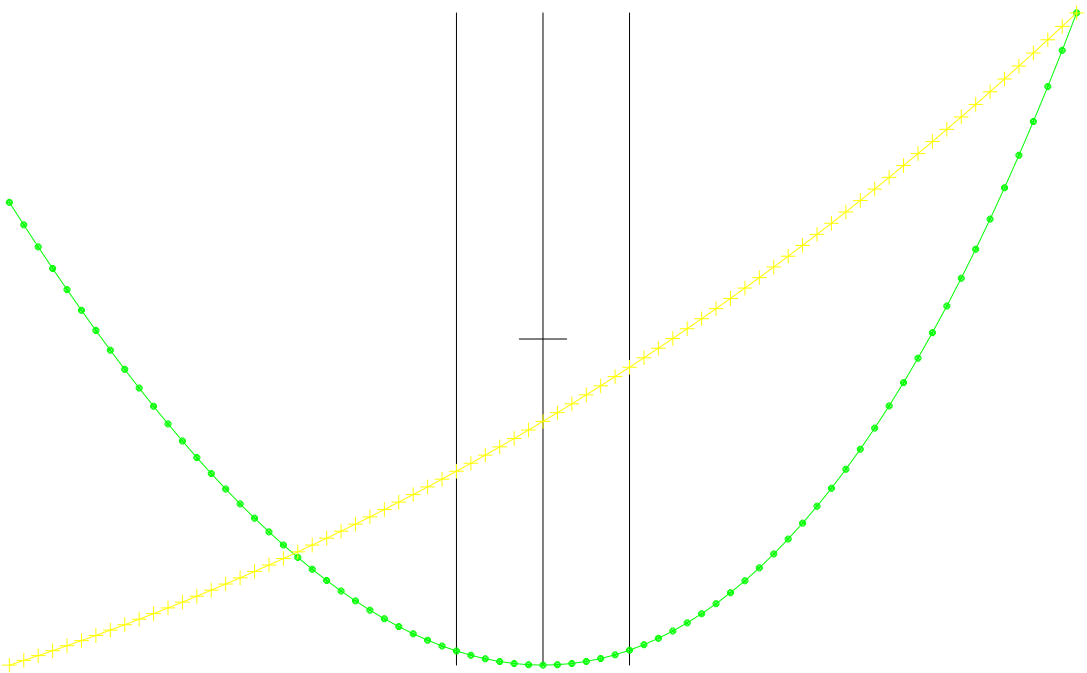

Point = 2.00 s = 2.50E-03
Direction = 1.000 h = 0.0150
F0 • (2.640E-11, 3.029E-03) F1 + (-0.04209, 0.07090)
Number of Evaluations: 418

This plot corresponding to figure

6