MICROSCOPE: A Software System for Multivariate Analysis

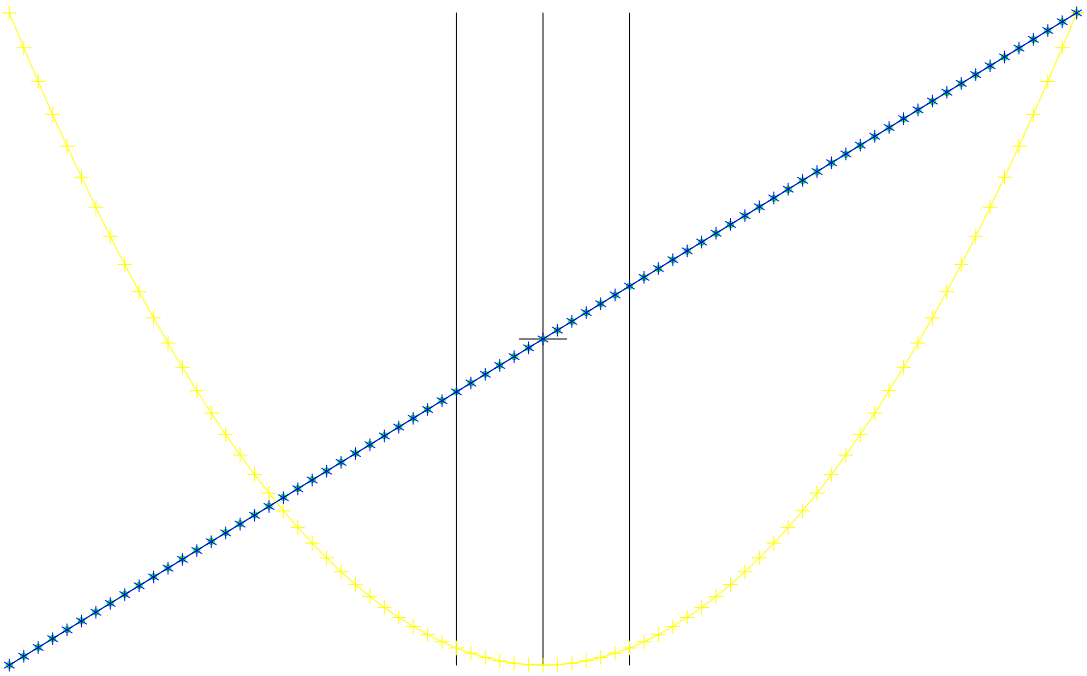

Point = 0.0
Direction = 1.000
F0 • (0.8828, 1.117)
F2 * (−0.2527, 0.2527)

s = 2.50E−03
h = 0.0150
F1 + (1.263, 1.275)
Number of Evaluations: 505

This plot corresponding to figure

7