MICROSCOPE: A Software System for Multivariate Analysis

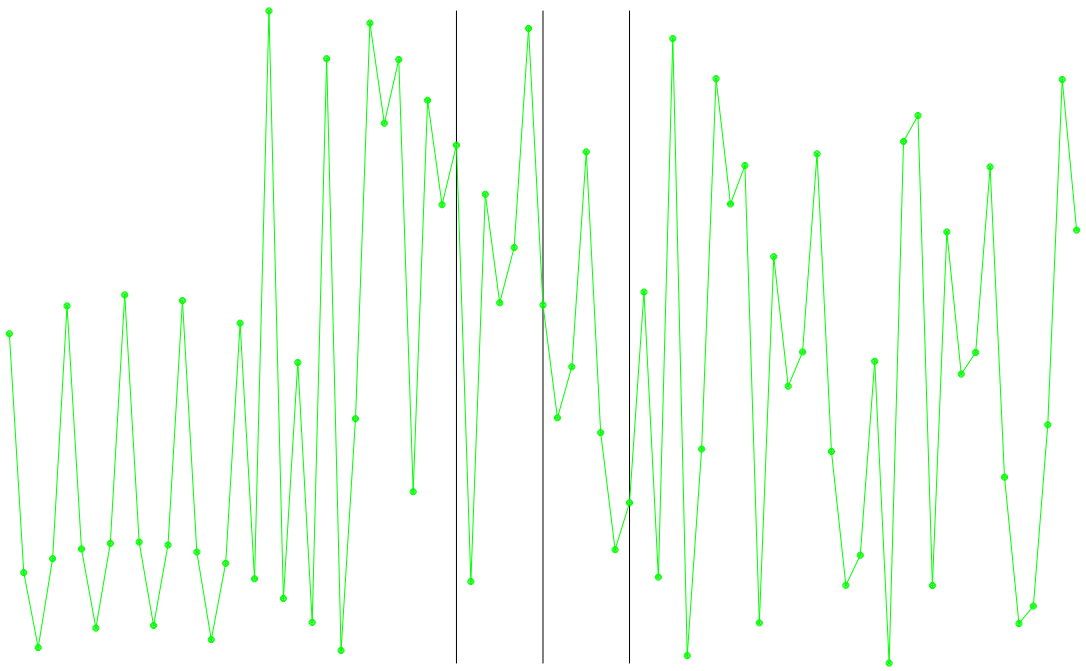

Point = 0.234 s = 2.50E-03
Direction = 1.000 h = 0.0150
F0 • (-9.993E-11, 9.781E-11) Number of Evaluations: 667

This plot corresponding to figure

9